


Test Report

System Type: **Mobile Air Ionizer**

Serial-No: **Example**

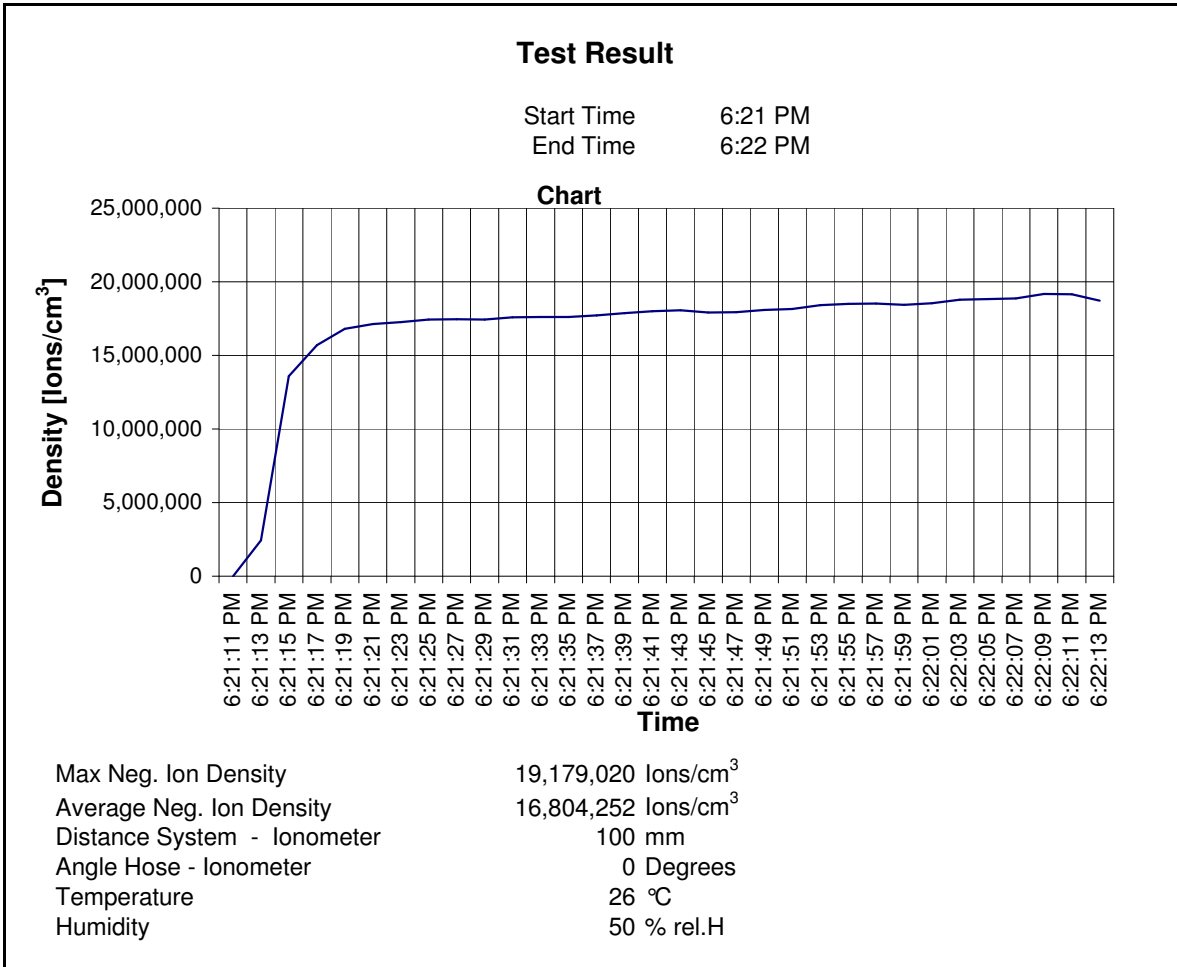

Test Equipment	
Ionometer IM806	Serial-no.: 74IM0138

Signature Tester

Important

The Air Ion density depends on the distance between the hose and the Ionometer.
 Change Filter every 200 hours to keep up the high performance of your AIR ENERGIZER